
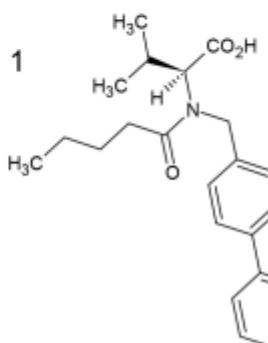


Standard solution*


(0.05 mg/mL Valsartan, 0.06 mg/mL Diclofenac sodium)

mAU

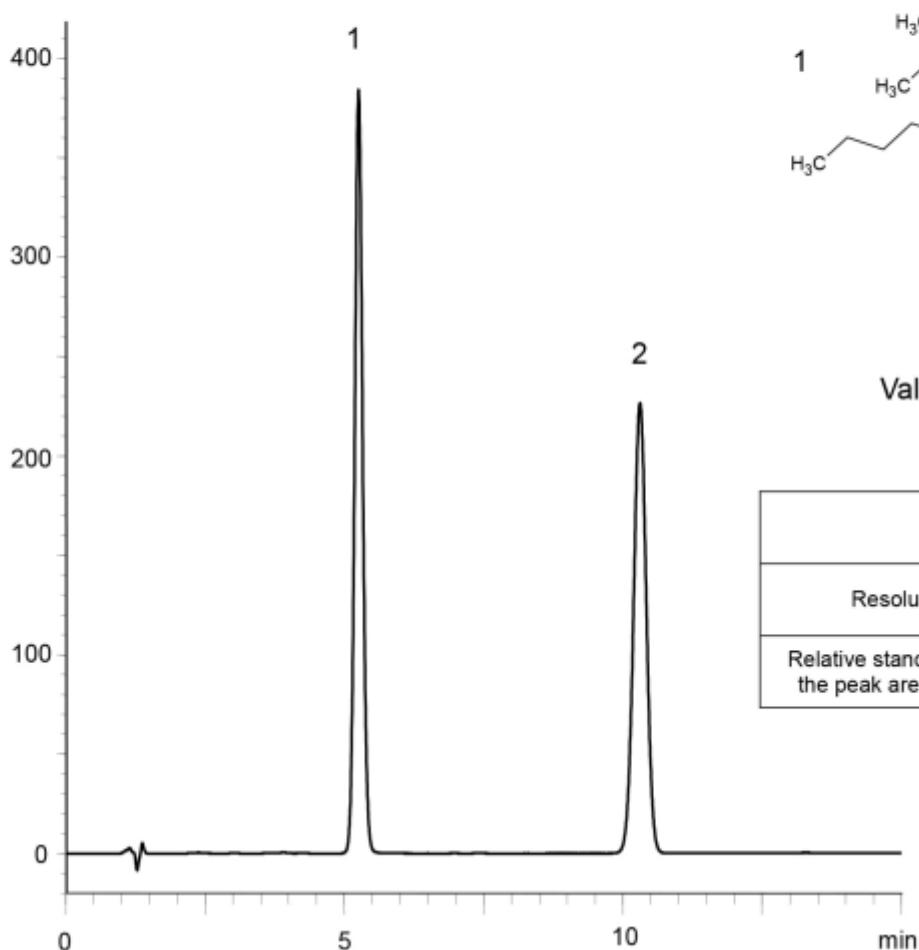

Valsartan

2



Diclofenac sodium (I.S.)

	System suitability requirement	Result
Resolution (1, 2)	≥5	14.9
Relative standard deviation of the peak area ratio of 1 to 2	≤1.0%	0.05%

Column	: YMC-Triart C18 (5 µm, 12 nm) 125 X 3.0 mmI.D.
Eluent	: acetonitrile/water/acetic acid (50/50/0.1)
Flow rate	: 0.45 mL/min (<i>adjust the flow rate so that the retention time of valsartan is about 5 min</i>)
Temperature	: 25°C
Detection	: UV at 225 nm
Injection	: 10 µL
(The draft for the Japanese Pharmacopoeia; Assay)	

* Standard solution was prepared from Valsartan supplied as a reagent for laboratory use.